

iMINI™ USB PDF

- Plug & Play single trip data logger
- No special software required
- Pre-programmed to customer specifications
- Compact profile; weightless than 14g
- Large memory capacity
- Long battery life
- 7 LED indicators
- Waterproof pouch



CERTIFICATIONS



21 CFR
Part 11



Product Specifications

(continued on back)

Description	Specifications
Product Code	MS-ST-S-8 MS-ST-S-8-P (Pharma Compliant)
Memory Options	8K, 7928 readings
Program Interval	5 seconds to 17 hours
Time Accuracy	± 1 hour per year
Sensor	Internal
Temperature Range	-40°C to +80°C (-104°F to +176°F)
Temperature Accuracy	±0.5°C (-40°C to -10°C), ±32.9°F (-104°F to +14°F); ±0.3°C (-10°C to +80°C), ±32.5°F (-50°F to +176°F)
Resolution	0.1 °C (32.18°F)
Sensor Response Time	T90 of 5 minutes in moving air
LCD Operating Range	N/A
Alarm Thresholds	4 thresholds; 2 red LEDs, 2 blue LEDs
Alarm Configuration	HIGH HIGH, HIGH, LOW & LOW LOW
Bookmark	Yes, maximum 8
Preprogram Option	Factory programmed
Start Option	Push button
Auto Restart	N/A
Start Delay	Yes, 1 minute to 99 days
Stop Option	Yes, stop button (can be disabled)
Size	68x37x5mm (without sleeve); 81x52x5mm (with sleeve)

Product Specifications

(continued from front)

Logger

Case Material	Plastic sleeve
IP Rating	3.0V
Resolution	IP 65
Warranty	1 trip

Certification and software


Calibration	3pt NIST traceable built into PDF (MS-ST-S-8-P only)
Certificates	ISO9001:2008, CE, RoHS
Battery Life	1 Year
Software	ConsolePlus
Default File Format	PDF, TXT, CVT & CSV
Data Export	TXT, CSV, CVT & PDF



 LL L H HH

MS-CD-300-8545
 21:22:45 06/11/2013

Device specification	
Product code	MS-ST-S-8-P
Serial Number	MS-CD-300-8545
H/W Version	Ver_2_08
Trip Remaining	No
Description	Cryopak Verification Tech.
Battery	100%
Original time zone	UTC: -1
Start	06/11/2013 19:44:45
Finish	06/11/2013 21:22:25/C
Start Delay	0m
Interval	10s
Readings	587
Temperature Range	-40 to +80 °C
High High Alarm	50.0 °C
High Alarm	40.0 °C
Low Alarm	30.0 °C
Low Low Alarm	25.0 °C

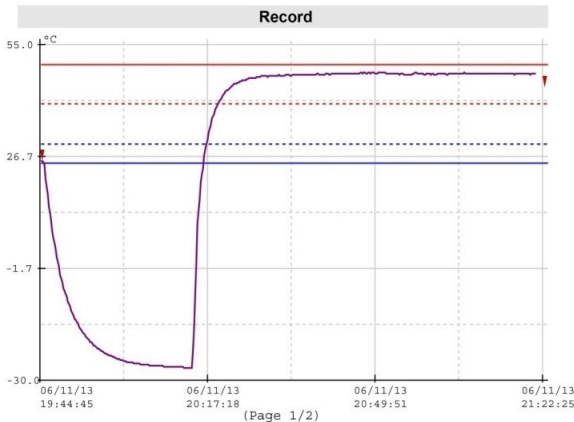



 LL L H HH

MS-CD-300-8545
 21:22:45 06/11/2013

Statistics	
Highest	48.0 °C
Average	26.2 °C
Lowest	-26.8 °C
High High Alarm	Enabled
High Alarm	Activated
Low Alarm	Activated
Low Low Alarm	Activated

Out of specification	
Above High High Alarm	00h00m00s
Above High Alarm	01h03m20s
Below Low Alarm	00h32m20s
Below Low Low Alarm	00h31m10s

21 CFR part 11 Compliant	
Security #	D285
ID-User name	#12-Saak Dertadian

Traceable Accuracy Certificate			
Certificate No	TT-MS-CD-300-8545		
Certificate Date	06/11/2013		
Certificate Validity	One Year or One Trip		
Reference	58.79°C	25.07°C	-19.53°C
Logger	58.79°C	25.30°C	-19.10°C
Variance	0.00°C	0.22°C	0.44°C
Pass / Fail	Pass	Pass	Pass
<small>S Range Temperature range: (-40°C to +80°C) Resolution: 0.1°C Traceable Accuracy: ±0.5°C (-40°C to -10°C), ±0.3°C (-10°C to +80°C)</small>			
<small>This product is certified using standards traceable to NIST. It has been tested and validated according to Cryopak's Standard Operating Procedures following guidelines set forth in ISO9001:2008. All temperatures are in degrees Celsius. These results do not incorporate the tolerance of the sensor. The associated uncertainty is 0.2</small>			

(Page 2/2)



United States

551 Raritan Center Parkway
Edison, NJ 08837

☎ 1.888.827.3393

Canada

11000 Parkway Blvd
Anjou, QC Canada H1J 1R6

☎ 1.888.423.7251

Europe

1 Rue Berthelot
Maromme, France 76150

☎ +33 2 32 82 59 65